



STRAUMANN® BLT/TL İMPLANT



Straumann® Sümük Səviyyəsi Konik İmplant

Straumann brendinin Sümük Səviyyəsi Konik implantları özünə məxsus dizaynı ilə bir çox üstünlükləri bir arada cəmləyir. BLT (Bone Level Tapered) implantın konik formada olması implantın yuvaya yerləşdirilməsi zamanı ilkin sabilliyin daha asan əldə olunmasını təmin edir.


Straumann® Sümük Səviyyəsi Konik İmplantlarının material və səthinə görə iki fərqli məhsul təqdim edir. Roxolid® SLActive® və Roxolid® SLA®.

İmplantlar, köməkçi və cərrahi parçalar implant ölçüsünə uyğun olaraq rənglər ilə kodlaşdırılıb.

Rəng kodları		
●	mavi	İmplant diametri 2.9 mm
●	sarı	İmplant diametri 3.3 mm
●	qırmızı	İmplant diametri 4.1 mm
●	yaşıl	İmplant diametri 4.8 mm

MATERIAL

Straumann® patenti özünə məxsus olan, tam yeni texnologiya ilə hazırlanan, dünya bazarında ilk və tək olan Roxolid® materialını təqdim edir. Bu material sayəsində Ø2.9 mm və 4 mm(h) implantların istehsalı mümkün olur. Roxolid® titanium və zirkonium birləşməsindən alınan və saf titaniumdan dəfələrlə daha sərt olan bir materialdır. Roxolid® materialının tərkibində Aliminium və Vanadium olmaması sayəsində implantın insan orqanizmində hər hansı allergik təsirinin qarşısı alınmış olur.

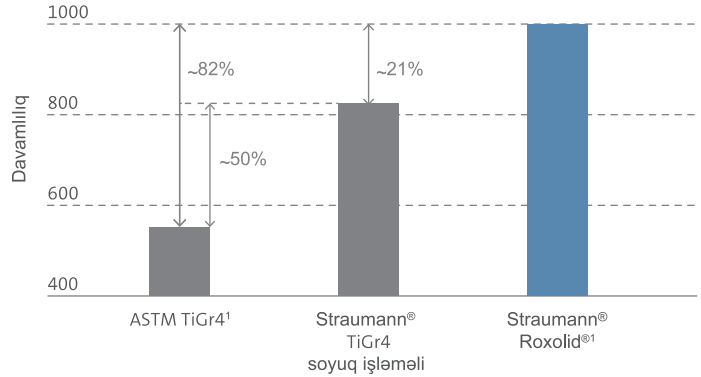


SƏTH

Straumann®-in ən müasir texnologiya ilə əldə etdiyi SLA (Sand blasted, Large grit, Acid etched) səthi bir biri ilə əlaqəli mikro yuvacıqlar sayəsində əldə etdiyi mükəmməl hidrofili xüsusiyyəti osteointeqrasiya prosesinin digər implantlar ilə müqayisədə iki dəfə daha sürətli baş verməsinə şərait yaradır.

Bununla kifayətlənməyən Straumann® öz patent texnologiyası ilə hazırladığı SLActive® səthini dünya bazarına təqdim edir. SLActive® səthli implantın aşağıdakı üstünlükləri var:

1. D2 sümükde osteointeqrasiya prosesinin 21-ci gündə bitməsi.
2. 60 yaş üzəri pasientlərdə uğurlu nəticələrin əldə olunması.
3. Onkoloji xəstələrdə uğurlu nəticələrin əldə olunması.
4. Şəkər xəstələrində uğurlu nəticələrin əldə olunması.
5. Riskli zonalarda uğurlu nəticələrin əldə olunması.

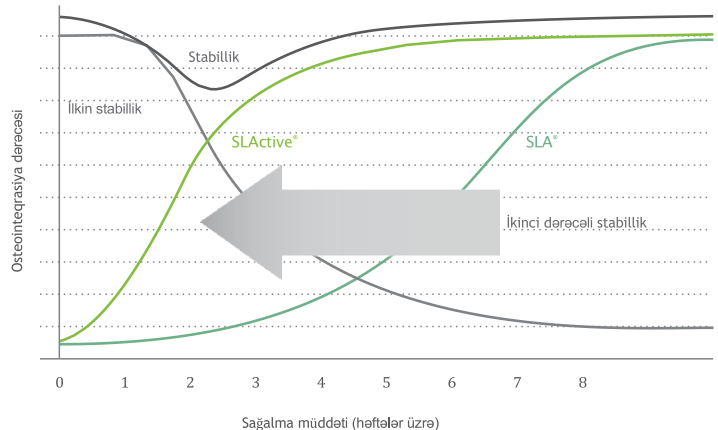

LOXİM

Straumann® implantlarının üzerinde Loxim® adlanan mavi r ngli bir hiss c k var ki, bunun k m kliyi  l  implantın qabından asanlıqla  ıxarılması m mk n olur. Bundan  lav , Loxim® hiss ciyinin 50 N/m t zyiqd  m rk zd n qırılması x susiy ti  m liyyat zamanı implantın normadan artıq sıxılması riskini aradan qaldırır v  nekroz kimi x      m z travmaların ba  verm sinin qar ısını alır. K narındaki n  t l r vasit si  l  biz implantın yuvadakı istiqam tinin t yin ed  bilirik. Loxim® texnologiyasının patenti Straumann® brendinə maxsusdur v  analoqu m vcud deyildir.





Alətlər

ALƏTLƏRİN ÖLÇÜLƏRİ

Straumann alətlərinin üzərində 2mm interval ilə ölçü həddləri mövcuddur.

Qalın xətt 10mm ilə 12 mm hədd aralığını bildirir.

Diqqət: Burğular uc hissədən etibarən implantdan 0.4mm daha uzundur.

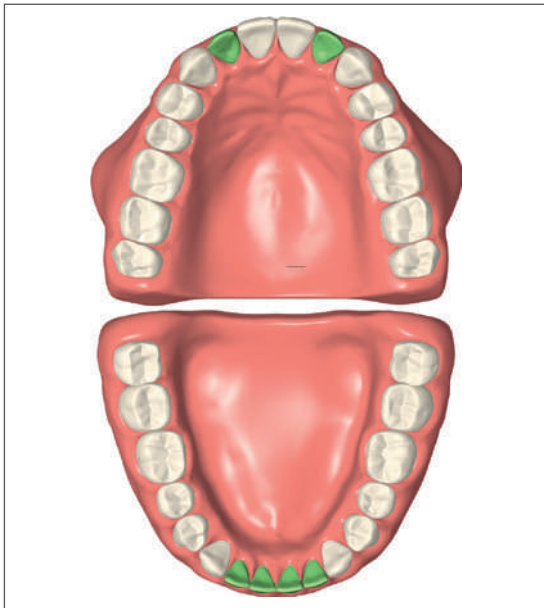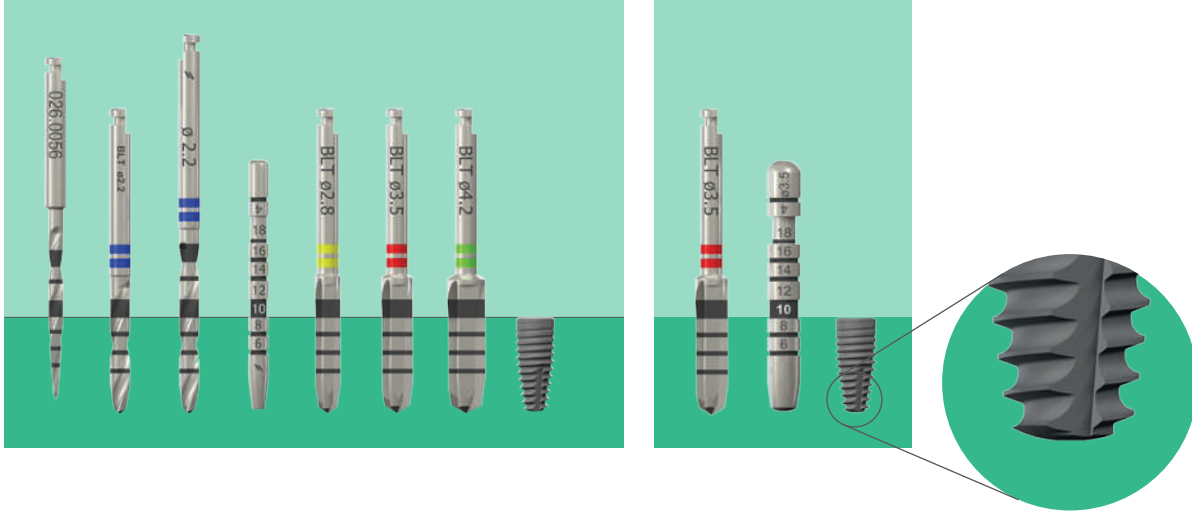


SÜMÜK SƏVIYYƏSİ KONİK Ø2.9MM İMPLANT

Straumann® BLT 2.9mm implant aşağıda qeyd olunan nahiyyələrdə təkli defektləri aradan qaldırmaq üçün nəzərdə tutulub.

- Mandibulyar mərkəzi və lateral kəsici dişlər.
- Maksillar lateral kəsici dişlər.
- Yalnız 0° bucaq altında yerləşdirilə bilər.


CƏRRAHİ PROSEDUR

Straumann® Ø2.9 mm Sümük Səviyyəsi Konik implant.

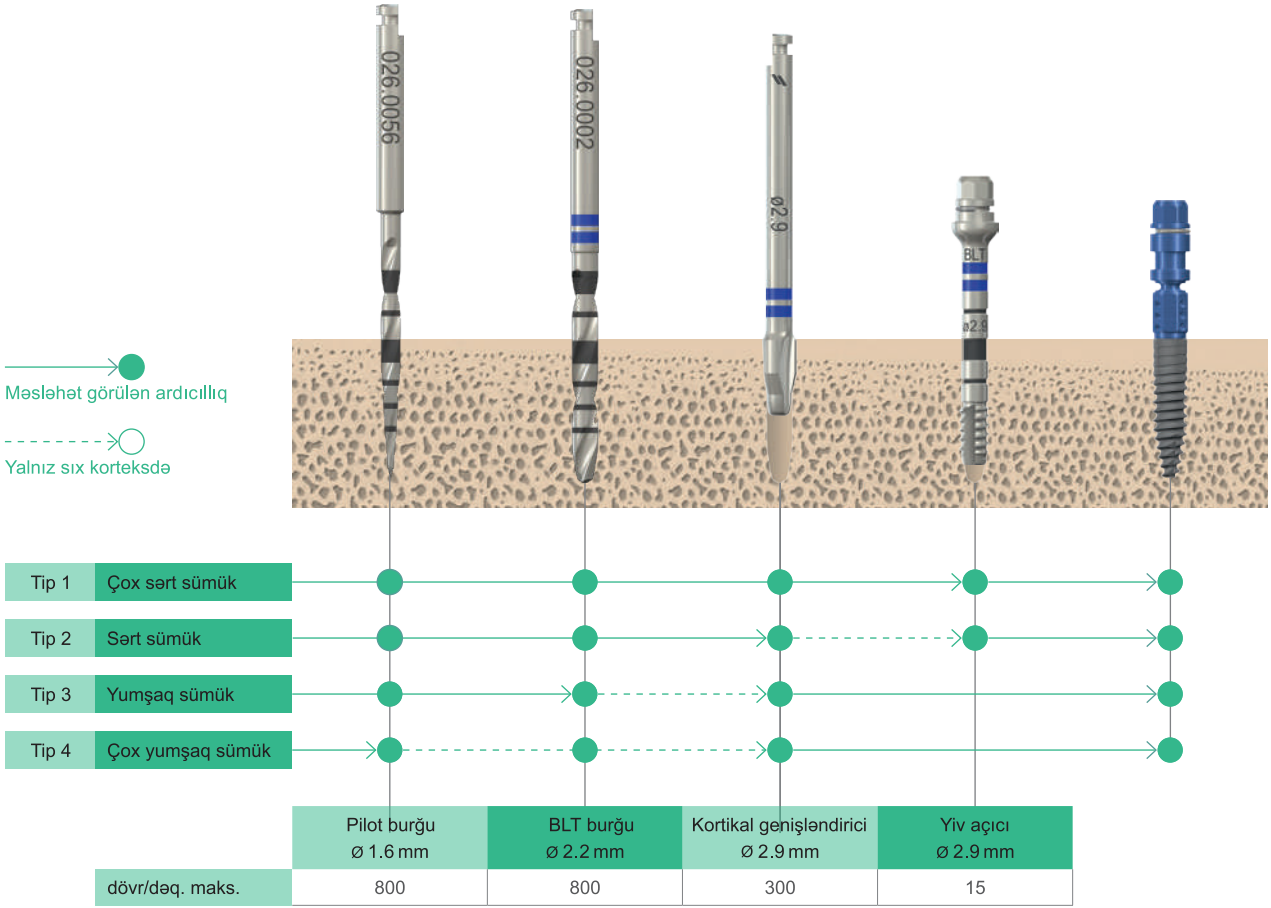


024.0006S		SC qapama vidası Ø 2.4 mm, H 0.5 mm, Ti
024.0007S		SC sağalma başlığı, konik, oval, H 2 mm, Ti
024.0008S		SC sağalma başlığı, konik, oval, H 3.5 mm, Ti
024.0009S		SC sağalma başlığı, konik, oval, H 5 mm, Ti
024.0010S		SC sağalma başlığı, konik, oval, H 6.5 mm, Ti

Straumann® Ø 3.3 mm Sümük Səviyyəsi Konik implant.

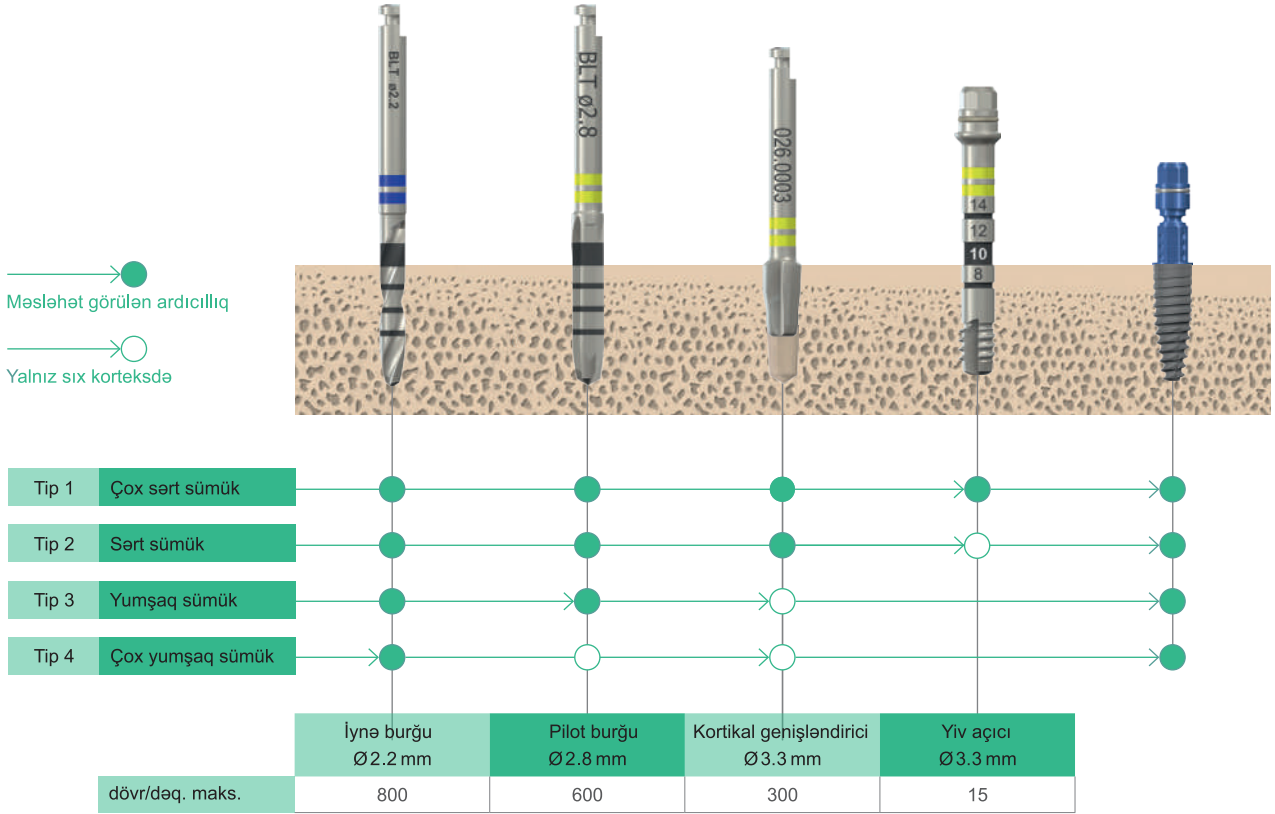

NC qapama vidası					
		small	0 mm	Ti	024.2100S
		packaging 4 pieces			024.2100S-04
NC sağalma başlığı					
		Ø 4.8 mm, conical	3,5 mm	Ti	024.2244S
			5 mm		024.2246S
		Ø 5 mm, customizable	7 mm	PEEK	024.2270S

Straumann® Ø4.1 mm Sümük Səviyyəsi Konik implant.

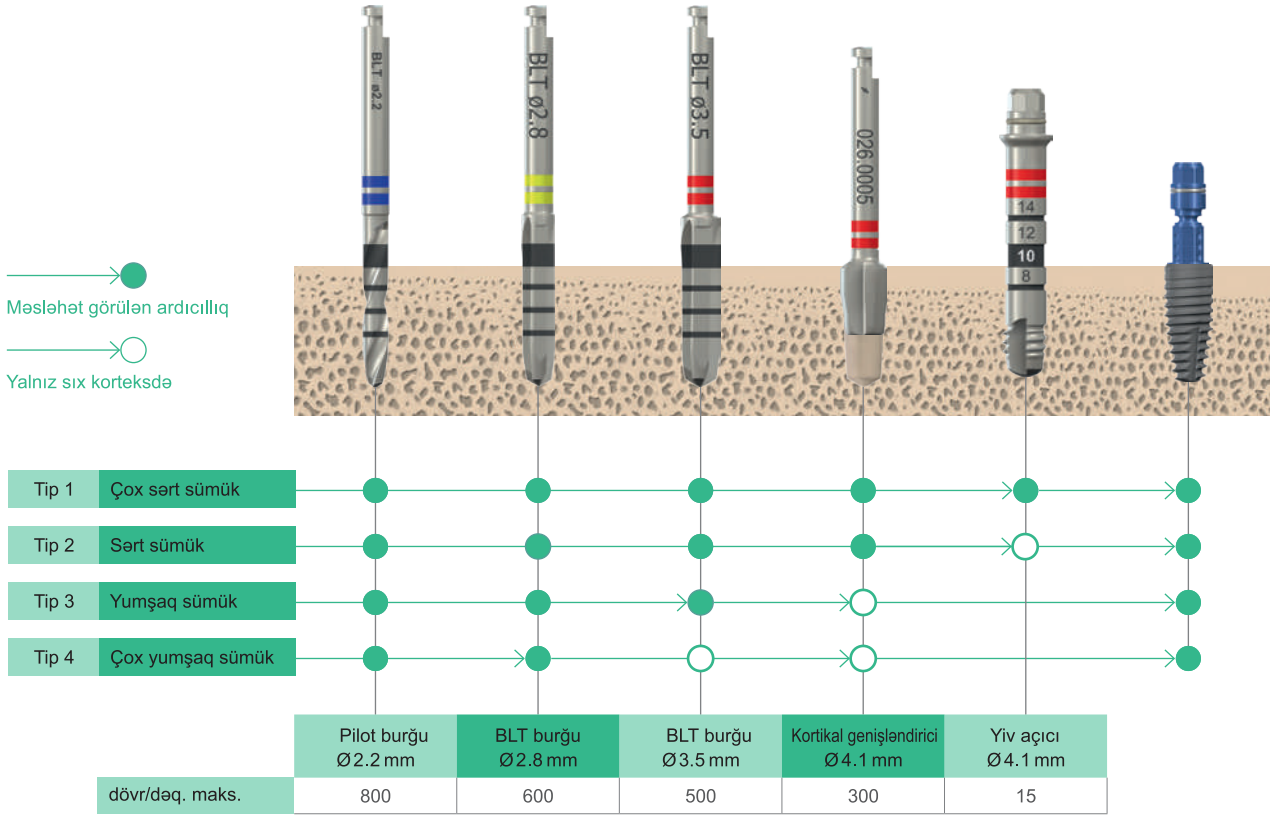


RC qapama vidası

	small	0 mm	Ti	024.41005
	packaging 4 pieces			024.41005-04

RC sağalma başlığı

	Ø 5 mm, conical	4 mm	Ti	024.4224S
		6 mm		024.4226S
	Ø 6.5 mm, conical	4 mm		024.4244S
		6 mm		024.4246S
	Ø 7 mm, customizable	7 mm	PEEK	024.4270S

Straumann® Ø4.8 mm Sümük Səviyyəsi Konik implant.

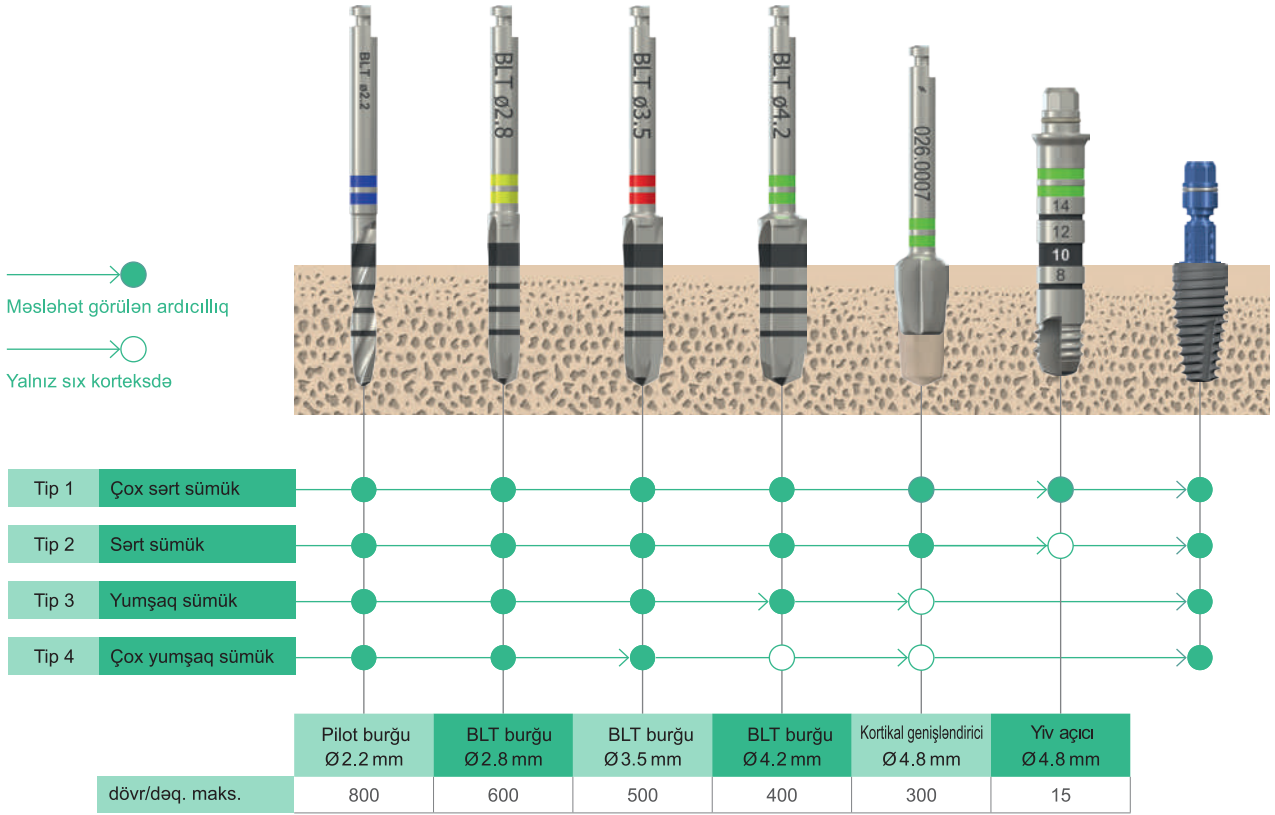

RC qapama vidası

		small	0 mm	Ti	024.4100S
		packaging 4 pieces			024.4100S-04
		large	0.5 mm		024.4105S
		packaging 4 pieces			024.4105S-04

RC sağalma başlığı

	Ø 5 mm, conical	4 mm	Ti	024.4224S
		6 mm		024.4226S
	Ø 6.5 mm, conical	4 mm		024.4244S
		6 mm		024.4246S
	Ø 7 mm, customizable	7 mm	PEEK	024.4270S

İMLANTIN YERLƏŞDİRİLMƏSİ

Straumann® implantları fiziodispenser və ya manual üsul ilə yuvaya yerləşdirilə bilər. Fiziodispenser ilə yerləşdirilmə zamanı məsləhət görülən sürət həddi 15 dövr/dəqiqədir.

İmplantın yuvaya yerləşdirilməsi aşağıda göstərilən ardıcılıq ilə tətbiq olunur.




Addım 1

İmplant daşıyıcı aləti mavi rəngli Loxim® hissəciyə "klik" səsinin müşayiəti ilə keçirilməlidir.




Addım 2

İmplant stabil formada daşıyıcı yuvadan çıxarılmalıdır.

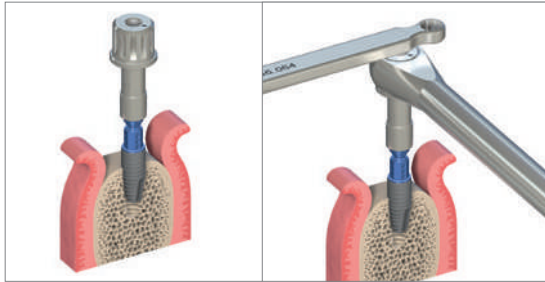


Addım 3

İmplantı yuvaya yerləşdirərkən ratçeti saat əqrəbi istiqamətində döndürmək lazımdır.

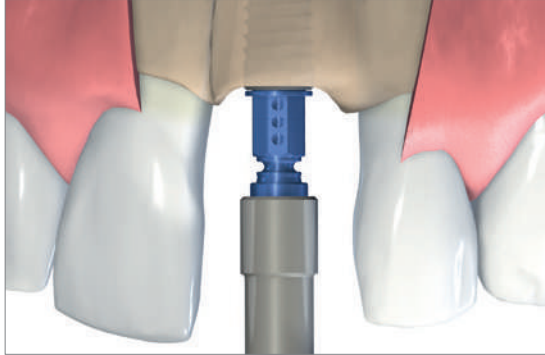

Addım 4

Yekun implant pozisiyasını təyin edərkən Loxim® hissəciyinin üzərindəki nöqtələr sizə kömək edəcəkdir. İmplant pozisiyasının doğru olması abatementin yüklənməsi mərhələsində arzulanan nəticəni əldə etməyə şərait yaradır.

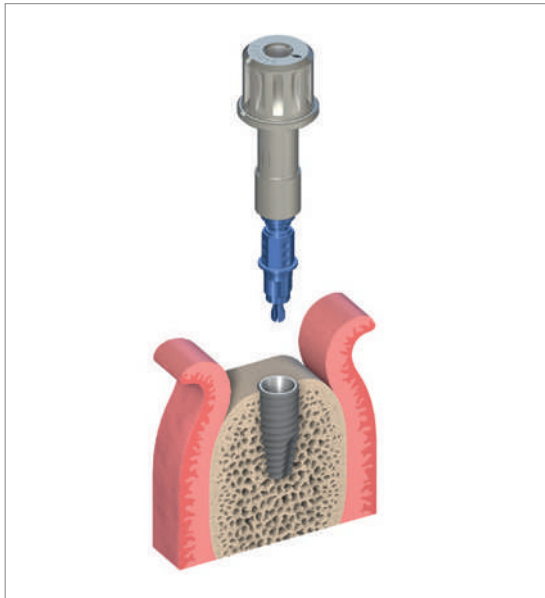


Addım 5

İmplant yuvaya tam olaraq yerləşdirildikdən sonra asanlıqla Loxim® hissəciyini implantdan çıxara bilərsiniz. Əgər, əməliyyat zamanı implant yuvadan geri çıxarılmalıdırsa ratçet vasitəsi ilə Loxim® hissəciyini saat əqrəbinin əksi istiqamətində döndürmək kifayətdir.

Roxolid® SLA® Implants

Bone Level Tapered Implants		NC	RC	RC	
		Ø 3.3 mm 	Ø 4.1 mm 	Ø 4.8 mm 	
SLA®		BLT Ø 3.3 NC	BLT Ø 4.1 RC	BLT Ø 4.8 RC	
8 mm		021.3508	021.5508	021.7508	
10 mm		021.3510	021.5510	021.7510	
12 mm		021.3512	021.5512	021.7512	
14 mm		021.3514	021.5514	021.7514	
16 mm		021.3516	021.5516	021.7516	

Roxolid® SLActive® Implants

Bone Level Tapered Implants	SC	NC	RC	RC	
	Ø 2.9 mm 	Ø 3.3 mm 	Ø 4.1 mm 	Ø 4.8 mm 	
SLActive®	BLT Ø 2.9 SC	BLT Ø 3.3 NC	BLT Ø 4.1 RC	BLT Ø 4.8 RC	
8 mm	-	021.3308	021.5308	021.7308	
10 mm	021.0010	021.3310	021.5310	021.7310	
12 mm	021.0012	021.3312	021.5312	021.7312	
14 mm	021.0014	021.3314	021.5314	021.7314	
16 mm	-	021.3316	021.5316	021.7316	

Impression-taking/Master Cast Fabrication

Product	Image	Description	Material	Art.-No.
Impression Posts and Analog				
SC Impression Post Open Tray, long		long, with guide screw, length 24 mm		025.0022
SC Impression Post Closed Tray		with 1 guide screw & 2 caps, length 19 mm	TAN/POM	025.0020
SC Implant Analog		length 11 mm	TAN	025.0023

Digital Impression				
SC CARES® Mono Scanbody		Ø 3.5 mm, height 10 mm	PEEK/TAN	025.0025
SC Repositionable Implant Analog		length 17 mm	Stainless steel	025.0024

Temporary Restorations

Product	Image	Description	Material	Art.-No.
Temporary Abutments				
SC Temporary Abutment		including screw 025.0031, crown, oval, gingiva height 1 mm	TAN	024.0011
		including screw 025.0031, crown, oval, gingiva height 2 mm		024.0015
		including screw 025.0031, crown, oval, gingiva height 3 mm		024.0016

Variobase® Abutments				
SC Variobase® for Crown		including screw 025.0031, oval, gingiva height 1 mm	TAN	022.0038
		including screw 025.0031, oval, gingiva height 2 mm		022.0039
		including screw 025.0031, oval, gingiva height 3 mm		022.0040

Straumann® BLT

MÜALİCƏ
GÜCÜNÜN
YENİ DÖNƏMİ



 **straumann**
simply doing more

Cement-Retained Restoration, Cementable Abutments

Product	Image	Description	Material	Art.-No.
Cementable Abutments with Emergence Profile Ø 5 mm				
NC Cementable Abutment		including screw 025.2908, Ø 5 mm, gingiva height 1 mm, abutment height 5.5 mm	Ti	022.2325
		including screw 025.2908, Ø 5 mm, gingiva height 2 mm, abutment height 5.5 mm		022.2326
		including screw 025.2908, Ø 5 mm, gingiva height 3 mm, abutment height 5.5 mm		022.2327

Cement-Retained Restoration, Anatomic Abutments

Product	Image	Description	Material	Art.-No.
VITA CAD-Temp®				
NC Temporary Abutment VITA CAD-Temp®		including screw 025.2908, height 11 mm, Ø 5 mm	PMMA/TAN	024.2372

Temporary Abutments				
NC Temporary Abutment		for crowns, including screw 025.2900, height 11 mm, Ø 3.5 mm	TAN	024.2371
		for bridges, including screw 025.2900, height 11 mm, Ø 3.5 mm		024.2375

Product	Image	Description	Material	Art.-No.
Anatomic Abutments, Titanium				
NC Anatomic Abutment		straight, including screw 025.2900, gingiva height 2 mm	Ti	022.2102
		straight, including screw 025.2900, gingiva height 3.5 mm		022.2104
		angled, angulation 15°, including screw 025.2900, gingiva height 2 mm		022.2152
		angled, angulation 15°, including screw 025.2900, gingiva height 3.5 mm		022.2154

Replacement Screw				
NC Basal Screw		for NC Anatomic Abutments, NC Variobase® for Crown and Variobase® C, NC Gold Abutments and NC Gold and Titanium Abutments for bars, length 7.9 mm	TAN	025.2900

Impression-taking/Master Cast Fabrication

Product	Image	Description	Material	Art.-No.
Impression Posts and Analog				
NC Impression Post		screw-retained, for open-tray impression, short, length 16.5 mm	TAN	025.2202
		screw-retained, for closed-tray impression, includes 2 caps, length 12.3 mm	TAN/POM	025.2201
NC Implant Analog		length 11 mm	TAN	025.2101

Digital Impression				
CARES® NC Mono Scanbody		including Fixation Screw, Ø 3.5 mm, height 10 mm	PEEK/TAN	025.2915
NC Repositionable Implant Analog		for fully digital and conventional workflow, length 17 mm	Stainless steel	025.2102

Screw-retained Restoration with Screw-retained Abutment, Abutments with new design, sterile

Product	Image	Description	Material	Art.-No.
Screw-retained Abutments 0°, new design, sterile				
NC Screw-retained Abutment		straight, angulation 0°, Ø 4.6 mm, gingiva height 1.5 mm, sterile		022.01285
		straight, angulation 0°, Ø 4.6 mm, gingiva height 2.5 mm, sterile		022.01295
		straight, angulation 0°, Ø 4.6 mm, gingiva height 3.5 mm, sterile		022.01305

Screw-retained Abutments 17°, new design, sterile				
NC Screw-retained Abutment		angled, angulation 17°, Ø 4.6 mm, gingiva height 2.5 mm, type A, sterile	TAN	022.01365
		angled, angulation 17°, Ø 4.6 mm, gingiva height 3.5 mm, type A, sterile		022.01385
		angled, angulation 17°, Ø 4.6 mm, gingiva height 4.5 mm, type A, sterile		022.01405
		angled, angulation 17°, Ø 4.6 mm, gingiva height 5.5 mm, type A, sterile		022.01425

Screw-retained Abutments 30°, new design, sterile				
NC Screw-retained Abutment		angled, angulation 30°, Ø 4.6 mm, gingiva height 3.5 mm, type A, sterile	TAN	022.01445
		angled, angulation 30°, Ø 4.6 mm, gingiva height 4.5 mm, type A, sterile		022.01465
		angled, angulation 30°, Ø 4.6 mm, gingiva height 5.5 mm, type A, sterile		022.01485

Cement or Screw-retained Restoration, Variobase®

Product	Image	Description	Material	Art.-No.
Variobase® Abutments				
1 NC Variobase® for Crown		including screw 025.2900, Ø 3.8 mm, height 3.5 mm, gingiva height 1 mm	TAN	n/a
		including screw 025.2900, Ø 3.8 mm, height 3.5 mm, gingiva height 2 mm		
		including screw 025.2900, Ø 3.8 mm, height 3.5 mm, gingiva height 3 mm		
		including screw 025.2900, Ø 3.8 mm, height 5.5 mm, gingiva height 1 mm		
		including screw 025.2900, Ø 3.8 mm, height 5.5 mm, gingiva height 2 mm		
		including screw 025.2900, Ø 3.8 mm, height 5.5 mm, gingiva height 3 mm		
NC Variobase® for Crown AS		including screw 025.0055, Ø 4.1 mm, height 5.5 mm, gingiva height 1 mm		
NC Variobase® for Bridge/Bar Cylindrical		including screw 025.2926 and Cementation Aid 2, Ø 4.5 mm, height 3.5 mm		
Variobase® for Bridge/Bar Cylindrical Coping for Screw-retained Abutments Ø 4.6 mm		for Screw-retained Abutments Ø 4.6 mm, including screw 023.4763 and Cementation Aid 3, Ø 5.1 mm, height 4 mm		
Digital Impression				
CARES® NC Mono Scanbody		including Fixation Screw, Ø 3.5 mm, height 10 mm	PEEK/TAN	025.2915
NC Repositionable Implant Analog		for fully digital and conventional workflow, length 17 mm	Stainless steel	025.2102

Cement-Retained Restoration, Cementable Abutments

Product	Image	Description	Material	Art.-No.
Cementable Abutments with Emergence Profile Ø 5 mm				
RC Cementable Abutment		including screw 025.4908, Ø 5 mm, gingiva height 1 mm, abutment height 5.5 mm	Ti	022.4325
		including screw 025.4908, Ø 5 mm, gingiva height 2 mm, abutment height 5.5 mm		022.4326
		including screw 025.4908, Ø 5 mm, gingiva height 3 mm, abutment height 5.5 mm		022.4327

Cement-Retained, Anatomic Abutments

Product	Image	Description	Material	Art.-No.
Anatomic Abutments, Titanium				
RC Anatomic Abutment		straight, including screw 025.4900, gingiva height 2 mm	Ti	022.4102
		straight, including screw 025.4900, gingiva height 3.5 mm		022.4104
		angled, angulation 15°, including screw 025.4900, gingiva height 2 mm		022.4152
		angled, angulation 15°, including screw 025.4900, gingiva height 3.5 mm		022.4154

Temporary Restoration

Product	Image	Description	Material	Art.-No.
VITA CAD-Temp®				
RC Temporary Abutment VITA CAD-Temp®		including screw 025.4908, height 12 mm, Ø 7 mm	PMMA/TAN	024.4372

Temporary Abutments				
RC Temporary Abutment		for crowns, including screw 025.4900, height 11 mm, Ø 4.5 mm	TAN	024.4371
		for bridges, including screw 025.4900, height 11 mm, Ø 4.5 mm		024.4375

Replacement Screw				
RC Basal Screw		for RC Anatomic Abutments, RC Variobase® for Crown and Variobase® C, RC Gold Abutments for Crown and RC Gold and Titanium Abutments for bars, length 7.9 mm	TAN	025.4900

Impression-taking/Master Cast Fabrication

Product	Image	Description	Material	Art.-No.
Impression Posts and Analog				
RC Impression Post		screw-retained, for open-tray impression, short, length 16.5 mm	TAN	025.4202
		screw-retained, for closed-tray impression, includes 2 caps, length 12.3 mm	TAN/POM	025.4201
RC Implant Analog		length 11 mm	TAN	025.4101

Digital Impression				
CARES® RC Mono Scanbody		including Fixation Screw, Ø 4.1 mm, height 10 mm	PEEK/TAN	025.4915
RC Repositionable Implant Analog		for fully digital and conventional workflow, length 17 mm	Stainless steel	025.4102



Screw-retained Restoration with Screw-retained Abutment, Abutments with new design, sterile

Product	Image	Description	Material	Art.-No.
Screw-retained Abutments 0°, new design, sterile				
RC Screw-retained Abutment		straight, angulation 0°, Ø 4.6 mm, gingiva height 1.5 mm, sterile	TAN	022.01325
		straight, angulation 0°, Ø 4.6 mm, gingiva height 2.5 mm, sterile		022.01335
		straight, angulation 0°, Ø 4.6 mm, gingiva height 3.5 mm, sterile		022.01345
Screw-retained Abutments 17°, new design, sterile				
RC Screw-retained Abutment		angled, angulation 17°, Ø 4.6 mm, gingiva height 2.5 mm, type A, sterile	TAN	022.01505
		angled, angulation 17°, Ø 4.6 mm, gingiva height 3.5 mm, type A, sterile		022.01525
		angled, angulation 17°, Ø 4.6 mm, gingiva height 4.5 mm, type A, sterile		022.01545
		angled, angulation 17°, Ø 4.6 mm, gingiva height 5.5 mm, type A, sterile		022.01565
Screw-retained Abutments 30°, new design, sterile				
RC Screw-retained Abutment		angled, angulation 30°, Ø 4.6 mm, gingiva height 3.5 mm, type A, sterile	TAN	022.01585
		angled, angulation 30°, Ø 4.6 mm, gingiva height 4.5 mm, type A, sterile		022.01605
		angled, angulation 30°, Ø 4.6 mm, gingiva height 5.5 mm, type A, sterile		022.01625

Cement or Screw-retained Restoration, Variobase®

Product	Image	Description	Material	Art.-No.
Variobase® Abutments				
RC Variobase® for Crown		including screw 025.4900, Ø 4.5 mm, height 3.5 mm, gingiva height 1 mm	TAN	n/a
		including screw 025.4900, Ø 4.5 mm, height 3.5 mm, gingiva height 2 mm		
		including screw 025.4900, Ø 4.5 mm, height 3.5 mm, gingiva height 3 mm		
		including screw 025.4900, Ø 4.5 mm, height 5.5 mm, gingiva height 1 mm		
		including screw 025.4900, Ø 4.5 mm, height 5.5 mm, gingiva height 2 mm		
		including screw 025.4900, Ø 4.5 mm, height 5.5 mm, gingiva height 3 mm		
RC Variobase® for Crown AS		including screw 025.0055, Ø 4.7 mm, height 5.5 mm, gingiva height 1 mm		
RC Variobase® for Bridge/Bar Cylindrical		including screw 025.2926 and Cementation Aid 2, Ø 4.5 mm, height 3.5 mm		
Variobase® for Bridge/Bar Cylindrical Coping for Screw-retained Abutments Ø 4.6 mm		for Screw-retained Abutments Ø 4.6 mm, including screw 023.4763 and Cementation Aid 3, Ø 5.1 mm, height 4 mm		

Digital Impression				
CARES® RC Mono Scanbody		including Fixation Screw, Ø 4.1 mm, height 10 mm	PEEK/TAN	025.4915
RC Repositionable Implant Analog		for fully digital and conventional workflow, length 17 mm	Stainless steel	025.4102

Screw-retained Restoration with Screw-retained Abutment

Product	Image	Description	Material	Art.-No.
Impression Posts (at abutment level) for Single Crown Restoration (engaging)				
Impression Posts for Open-tray Impression		for Screw-retained Abutments, abutment level, Ø 3.5 mm	TAN	025.2243
		for Screw-retained Abutments, abutment level, Ø 4.6 mm		025.2244
Impression Posts for Closed-tray Impression		for Screw-retained Abutments, abutment level, Ø 3.5 mm	TAN/POM	025.2245
		for Screw-retained Abutments, abutment level, Ø 4.6 mm		025.2246

Impression Posts (at abutment level) for Multi-Unit Restorations (non engaging)				
Impression Posts for Closed-tray Impression		for Screw-retained Abutments, abutment level, Ø 4.6 mm	TAN/POM	025.0014

Digital Impression				
CARES® Mono Scanbody		for Screw-retained Abutments, abutment level, including Fixation Screw, Ø 3.5 mm	PEEK	025.0000
		for Screw-retained Abutments, abutment level, including Fixation Screw, Ø 4.6 mm		025.0001
Repositionable Analog		for Screw-retained Abutments, Ø 4.6 mm	Stainless steel	025.0008

Analog				
Analog for Screw-retained Abutments Ø 4.6 mm		for Screw-retained Abutments Ø 4.6 mm, straight	TAN	023.4756
		for Screw-retained Abutments Ø 4.6 mm, angled, angulation 17°/30°		023.4757

Roxolid® SLA®

Tissue Level RN		RN	RN	RN	
		Ø 3.3 mm  	Ø 4.1 mm  	Ø 4.8 mm  	
SLA®		TL Ø 3.3 RN	TL Ø 4.1 RN	TL Ø 4.8 RN	
6 mm		-	043.1615	043.0665	
8 mm		043.2605	043.1625	043.0675	
10 mm		043.2615	043.1635	043.0685	
12 mm		043.2625	043.1645	043.0695	
14 mm		043.2635	043.1655	043.0705	

Roxolid® SLActive®

Tissue Level RN		RN	RN	RN	
		Ø 3.3 mm  	Ø 4.1 mm  	Ø 4.8 mm  	
SLActive®		TL Ø 3.3 RN	TL Ø 4.1 RN	TL Ø 4.8 RN	
4 mm		-	033.0435	033.0445	
6 mm		-	033.5605	033.5905	
8 mm		033.5115	033.5615	033.5915	
10 mm		033.5125	033.5625	033.5925	
12 mm		033.5135	033.5635	033.5935	
14 mm		043.0705	033.5645	033.5945	

RN Closure Caps and Healing Caps

Product	Image	Description	Height	Material	Art.-No.
Closure Caps					
Sterile RN Closure Cap		Ø 3.5 mm, small	0 mm	Ti	048.371S

Healing Caps					
Sterile RN Healing Cap		Ø 5.5 mm	2 mm	Ti	048.033S
			3 mm		048.034S
			4,5 mm		048.037S

Impression-taking/Master Cast Fabrication

Product	Image	Description	Material	Art.-No.
Impression-taking (at implant level)				
RN Impression Post for open-tray impression		screw-retained, height 11 mm	Al/Ti	048.010
		screw-retained, height 21 mm		048.090
RN Impression Post for closed-tray impression		screw-retained, height 11 mm, with 1 guide screw & 2 caps	Al/Ti/POM	048.862

Analog				
RN Analog		gray with red stripe, length 12 mm	Stainless steel	048.124

Digital Impression				
CARES® RN Mono Scanbody		including Fixation Screw, Ø 4.8 mm, height 10 mm	PEEK/TAN	048.168
RN Repositionable Implant Analog		for fully digital and conventional workflow, length 17.6 mm	Stainless steel	048.129

Cement or Screw-retained Restoration, Angled Abutments

Product	Image	Description	Material	Art.-No.
Angled Abutments, 15°				
RN synOcta® Angled Abutment, 15°			Ti/TAN	
		long, type A, height 6.7 mm, with integral basal screw		048.610
				
		long, type B, height 6.7 mm, with integral basal screw		048.611
				048.605

Angled Abutments, 20°				
RN synOcta® Angled Abutment, 20°			Ti/TAN	
		long, type A, height 6.7 mm, with integral basal screw		048.615
				
		long, type B, height 6.7 mm, with integral basal screw		048.616
RN Variobase® for Crown		including screw 048.356, Ø 5.05 mm, height 6 mm		022.0022
RN synOcta® 1.5 Screw-retained Abutment		with integral basal screw, height 1.5 mm		048.601
RN synOcta® Plastic Coping		for synOcta® 1.5, for crowns, height 10 mm	POM	048.229
		for synOcta® 1.5, for bridges and bars, height 10 mm		048.227

Burn-out Copings				
Extension Shell		for synOcta® Angled Abutment, short and long 15° and 20°, height 5.5 mm	POM	048.670
Plastic Shoulder		for synOcta® Angled Abutment, short and long 15° and 20°, height 4 mm, packaging 4 pieces		048.676V4

Auxiliary Parts and Screws				
SCS Occlusal Screw		for occlusal screw-retained RN/WN Caps and Copings, length 4.4 mm	Ti	048.350

adentta

Ünvan: Həsən Əliyev 82 F, Bakı, Azərbaycan

Tel: (+994) 12 525 11 17

Mob: (+994) 55 409 98 78

Email: info@adentta.az

   adentta.az

Straumann BLT/TL implantları yüksək dəqiqlik, ilkin sabitlik və uzunmüddətli etibarlılıq təmin etmək məqsədilə hazırlanmışdır. Dünya üzrə minlərlə stomatoloqun seçimidir və klinik uğurlar, innovasiya və pasiyent məmnuniyyəti ilə seçilir.